



Application


Details of HPLC Application No. 116

Nucleosides on CS-ODS-5 μ

Column: 150 x 4,6 mm CS-ODS 100-5 μ

P/N: 586 1310 15

HPLC Conditions: Eluent: Water
Flow: 1,3 mL/min
Temperature: RT
Detector: UV 254 nm

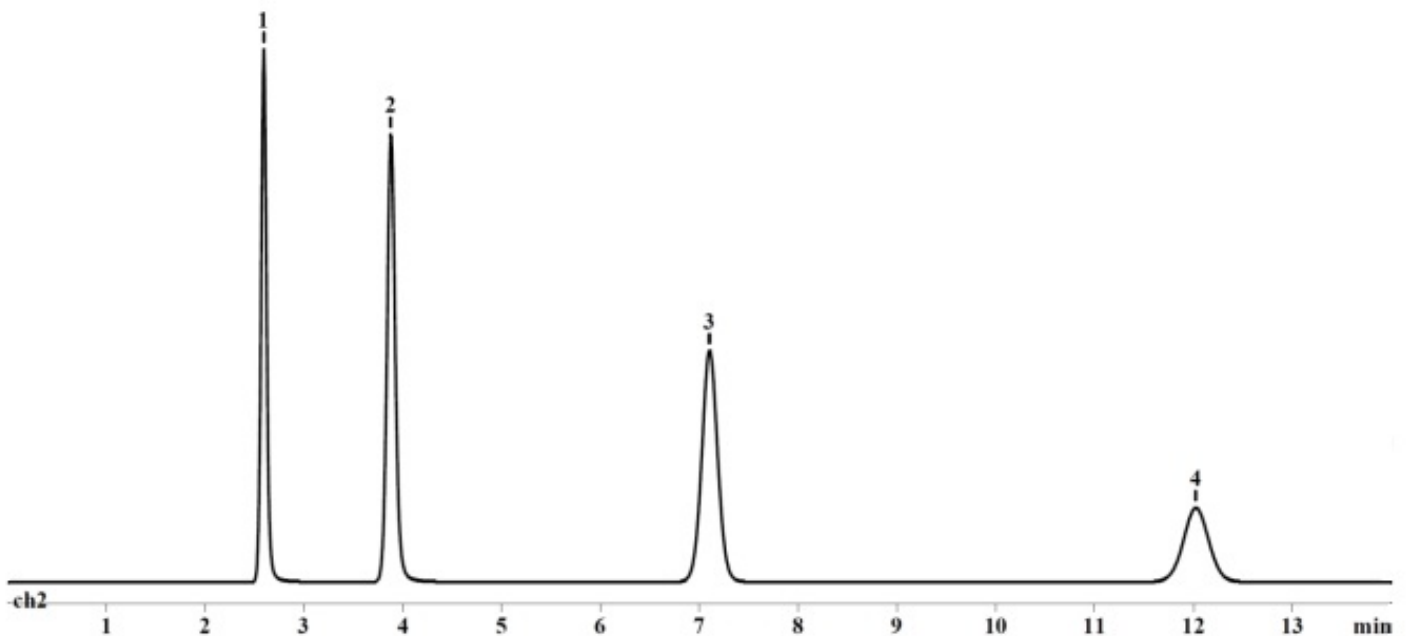

1.) Cytosine
2.) Uracil

3.) Cytidine
4.) Uridine

Peaks: Cytosine
Uracil
Cytidine
Uridine